


# RADIOCHEMISTRY

## List of Acronyms

<i>A</i>	<i>Standard Methods</i>	<i>NERHL</i>	<i>North Eastern Health Radiological Laboratory</i>
<i>ASTM</i>	<i>American Society for Testing &amp; Materials</i>	<i>NORM</i>	<i>Naturally Occurring Radioactive Materials</i>
<i>E or EPA</i>	<i>US Environmental Protection Agency</i>	<i>MDC</i>	<i>Minimum Detection Concentration</i>
<i>HNO<sub>3</sub></i>	<i>Nitric Acid</i>	<i>SW</i>	<i>Solid Waste – 846</i>
<i>LAACC</i>	<i>Large Area Activated Charcoal Canister</i>	<i>TSP</i>	<i>Total Suspended Particulate</i>
<i>HASL</i>	<i>Health and Safety Laboratory</i>	<i>USNRC</i>	<i>U.S. Nuclear Regulatory Commission</i>

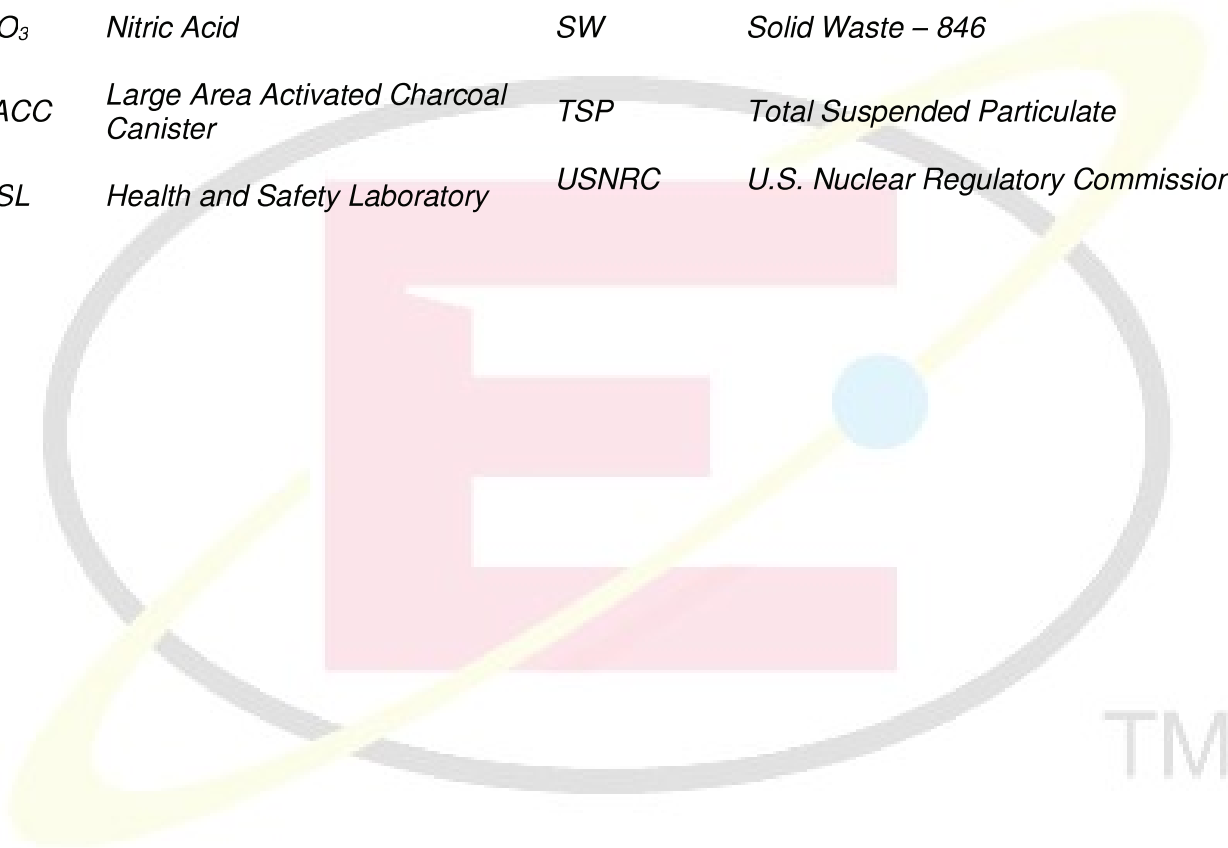

# RADIOCHEMISTRY

## 1. MATRIX DIGESTIONS – Prior to analysis

MATRIX	PREPARATION TECHNIQUE	AMOUNT OF SAMPLE REQUIRED
Drinking Water	HNO <sub>3</sub> to pH <2	1000 mL plastic
Drinking Water – <sup>222</sup> Radon	None Required	40 mL VOA vial – no headspace
Mine and Process Water – Soluble Constituents	Filtration, HNO <sub>3</sub> to pH <2	2000 mL plastic
Mine and Process Water – Total Constituents	HNO <sub>3</sub> to pH <2	2000 mL plastic
Solids – Core, Sediments, Sludges, Soils, Rock	Acid Digestion	100 g
Vegetation – USNRC Guidelines	Ashing, Acid Digestion	20 Kg
Biomass – USNRC Guidelines	Ashing, Acid Digestion	20 Kg
Air Filters	Acid Leaching	Filter sample and blank filter
Oils	Acid Leaching	100 g
Sample Preparation	Drying, Pulverizing	500 g
Sample Preparation	Canning	500 g

## 2. RADIOCHEMICAL ANALYSES – Drinking Water

ANALYSIS	METHOD	Drinking Water MCL	MIN. REQUIRED REPORTING LIMIT	UNITS
Gamma Emitting Radionuclides	E901.1	NA	dependent on sample size	pCi/L
Gross Alpha and Beta Radioactivity	E900.0	15/50 (see note)	3.0/4.0	pCi/L
Gross Radium Alpha (minus Radon & Uranium)	E900.1	15	3	pCi/L
<sup>226</sup> Radium (Alpha Emitting Isotopes)	E903.0	5.0 (see note)	1	pCi/L
<sup>228</sup> Radium (Beta Emitting Isotopes)	RA-05	5.0 (see note)	1	pCi/L
<sup>222</sup> Radon	ASTM D5072-92	NA	100	pCi/L
Isotopic Uranium ( <sup>234</sup> U, <sup>235</sup> U, <sup>238</sup> U)	E908.0	NA	0.67	pCi/L
Uranium	E200.8	30	1	ug/L
<b>Sample Location:</b> Entry point to distribution				
<b>Notes:</b>				
Gross Beta Activity MCL = 4 mRem/year ~ = 50 pCi/L. Regulation specifies monitoring for vulnerable systems.				
The Radium MCL is for a combined Radium 226+Radium 228 = 5.0 pCi/L.				

# RADIOCHEMISTRY

## 3. RADIOCHEMICAL ANALYSES - Applicable to most matrices listed above (after digestion)

Reporting Limits are matrix dependent

ANALYSIS	METHOD	MIN. REQUIRED REPORTING LIMIT	UNITS
Gamma Emitting Radionuclides	E901.1	dependent on sample size	pCi/L
Gross Alpha and Beta Radioactivity	E900.0	1.0/2.0	pCi/L
Gross Radium Alpha (minus Radon & Uranium)	E900.1	1	pCi/L
<sup>210</sup> Lead	E909.0	1	pCi/L
<sup>210</sup> Polonium	HASL-300 Po-02-RC	1	pCi/L
<sup>40</sup> Potassium	E901.1	dependent on sample size	pCi/L
<sup>226</sup> Radium (Alpha Emitting Isotopes)	E903.0	0.2	pCi/L
<sup>228</sup> Radium (Beta Emitting Isotopes)	RA-05	1	pCi/L
<sup>222</sup> Radon	ASTM D5072-92	100	pCi/L
Isotopic Thorium ( <sup>228</sup> Th, <sup>230</sup> Th, <sup>232</sup> Th)	E908.0	0.2 per Isotope	pCi/L
<sup>232</sup> Thorium	E200.8/SW6020	1	pCi/L
Isotopic Uranium ( <sup>234</sup> U, <sup>235</sup> U, <sup>238</sup> U)	A7500-U-C	0.2 per Isotope	pCi/L
Uranium, natural	E200.8/SW6020	0.2	pCi/L
Uranium, natural – low level	E200.8/SW6020	-	pCi/L

## 4. BIOASSAY - Uranium and other radionuclides in urine per USNRC Guideline 8.22.

ANALYSIS	REQUIRED VOLUME, mL	QC REQUIRED	MIN. REQUIRED REPORTING LIMIT	UNITS
Isotopic Uranium	1000 plastic	client specific	0.1	pCi/L
Uranium	100 plastic	25%	5	µg/L

# RADIOCHEMISTRY

## 5. RADIOLOGICAL FIELD SERVICES

SERVICE	
Radon - inside air by charcoal canister method (Ramses II Detector)	by Quote
Consulting Radiation Safety Officer – USNRC Accepted	by Quote
Surface Gamma Surveys - baseline, decontamination and decommissioning, process operations	by Quote
Air Quality Sampling - TSP, High Volume Air Sampling	by Quote
Equipment Decontamination and Release Surveys	by Quote
Emanation Coefficient	by Quote
Naturally Occurring Radioactive Materials (NORM) Surveys – oilfield related	by Quote
Large Area Activated Charcoal Canister (LAACC) Tailings Surveys - Radon Flux by Method E115	by Quote
Indoor Radon and Radon Progeny Measurements – Single or Multiple Site	by Quote
Custom Radiation Safety Courses - mining, milling, and reclamation projects	by Quote

TM